



# ARROW® PICC Set

4 Fr. | 55 cm catheter length

.018 inch dia. guide wire

80 cm Hydrophilic-Coated Nitinol Guidewire

Distal Lumen  
ARROW® VPS®  
Compatible

## REF PR-35541-HPHNM

### Contents:

- ① 1: Indwelling TaperFree™ Catheter: 4 Fr. x 55 cm **Pressure Injectable** Radiopaque Polyurethane with Blue FlexTip®, Extension Line Clamp, and Contamination Guard
- ② 1: GlideThru™ Peel-Away Sheath: 4 Fr. x 4" (10 cm) Radiopaque over 4 Fr. Dilator
- ③ 1: **Guidewire, Marked: .018" (0.46 mm) dia. x 80 cm Hydrophilic-Coated Nitinol with Soft Tip Tungsten Coil** (CE 0120)
- ④ 1: Guidewire, Marked: .018" (0.46 mm) dia. x 17-3/4" (45 cm) Nitinol (Straight Soft Tip on One End – Straight Stiff Tip on Other)
- ⑤ 1: Introducer Needle: Echogenic 21 Ga. x 2-3/4" (7 cm) TW
- ⑥ 1: Syringe: 10 mL Luer-Lock
- ⑦ 1: Skin Protectant Prep Pad
- ⑧ 1: Dust Cap: Non-Vented
- ⑨ 1: SecondSite™ Adjustable Hub: Catheter Clamp and Fastener
- ⑩ 1: **Catheter Trimmer**
- ⑪ 1: **Safety Scalpel: #11**
- ⑫ 1: Chart Sticker
- ⑬ 1: Checklist/CLIP Sheet
- ⑭ 1: Flow Rate Information Card with Injection Log
- ⑮ 1: Patient ID Card
- ⑯ 1: Patient Information Booklet
- ⑰ 1: **Dressing: STATLOCK®† Catheter Stabilization Device**
- ⑱ 1: Paper Tape Measure

† A registered trademark of C. R. Bard, Inc.

All components are CE 0086 unless otherwise noted.



Caution



Do not reuse



Do not resterilize



Sterilized  
by ethylene oxide



Keep away  
from sunlight



Keep dry



Do not use if  
package is damaged



Is not made with  
natural rubber latex



Consult  
instructions for use





Rx only. Warning: Read all package insert warnings, precautions, and instructions prior to use. Failure to do so may result in severe patient injury or death.

Sterile. Fluid path components are non-pyrogenic. Contains no medication.

**ARROW**  
INTERNATIONAL  
2400 Bernville Road  
Reading, PA 19605 USA  
[www.arrowintl.com](http://www.arrowintl.com)



Teleflex Medical  
IDA Business and  
Technology Park  
Dublin Road, Athlone  
Co. Westmeath, Ireland

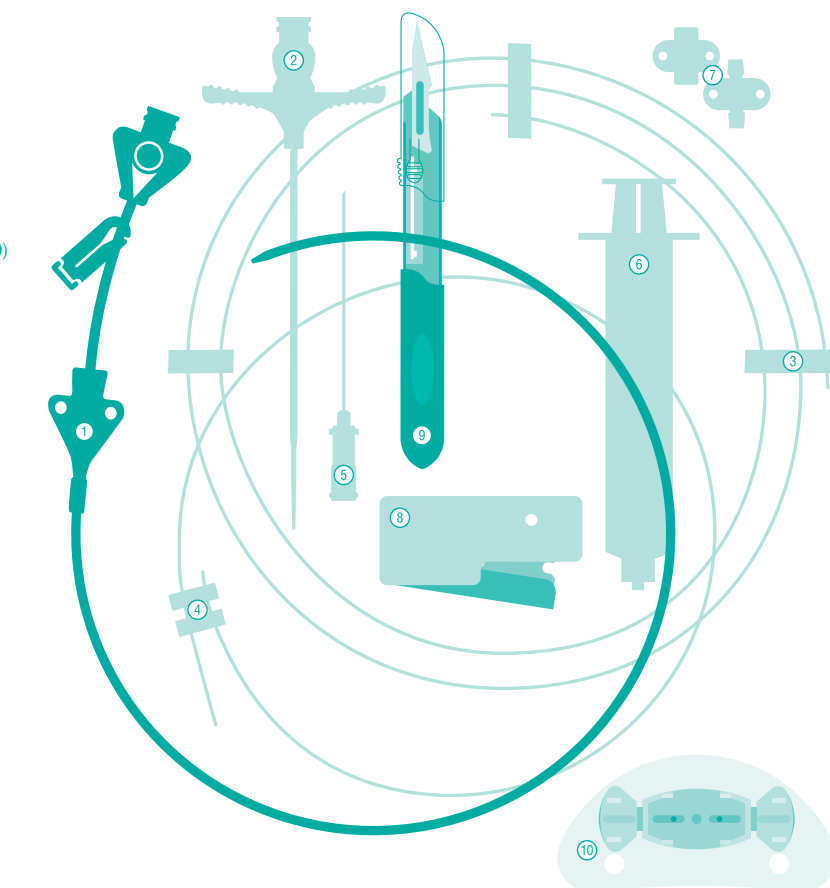

Lumen	Priming Volume* (mL)	Flow Rate† (mL/hr)	Pump Flow Rate‡ (mL/hr)	MAX Pressure Injection Flow Rate** (mL/sec)
Distal (17 Ga.)	0.58	1140	5720	5

\* Priming volumes are approximate and are done without injection caps.

† Flow rates were determined using room temperature water, 100 cm head height and represent approximate flow capabilities.

‡ Pump flow rates are determined at maximum pump pressure of 10 psig and represent approximate flow capabilities.

\*\*Pressure injection flow rates are determined at the injector pressure setting of 300 psi maximum using media of 11.8 centipoise viscosity, with 152 cm pressure tubing.